


Scan: 50.00 - 450.00 Samples: 64 Thresh: 0 Step: 0.10  
536 peaks Base: 385.50 Abundance: 2499

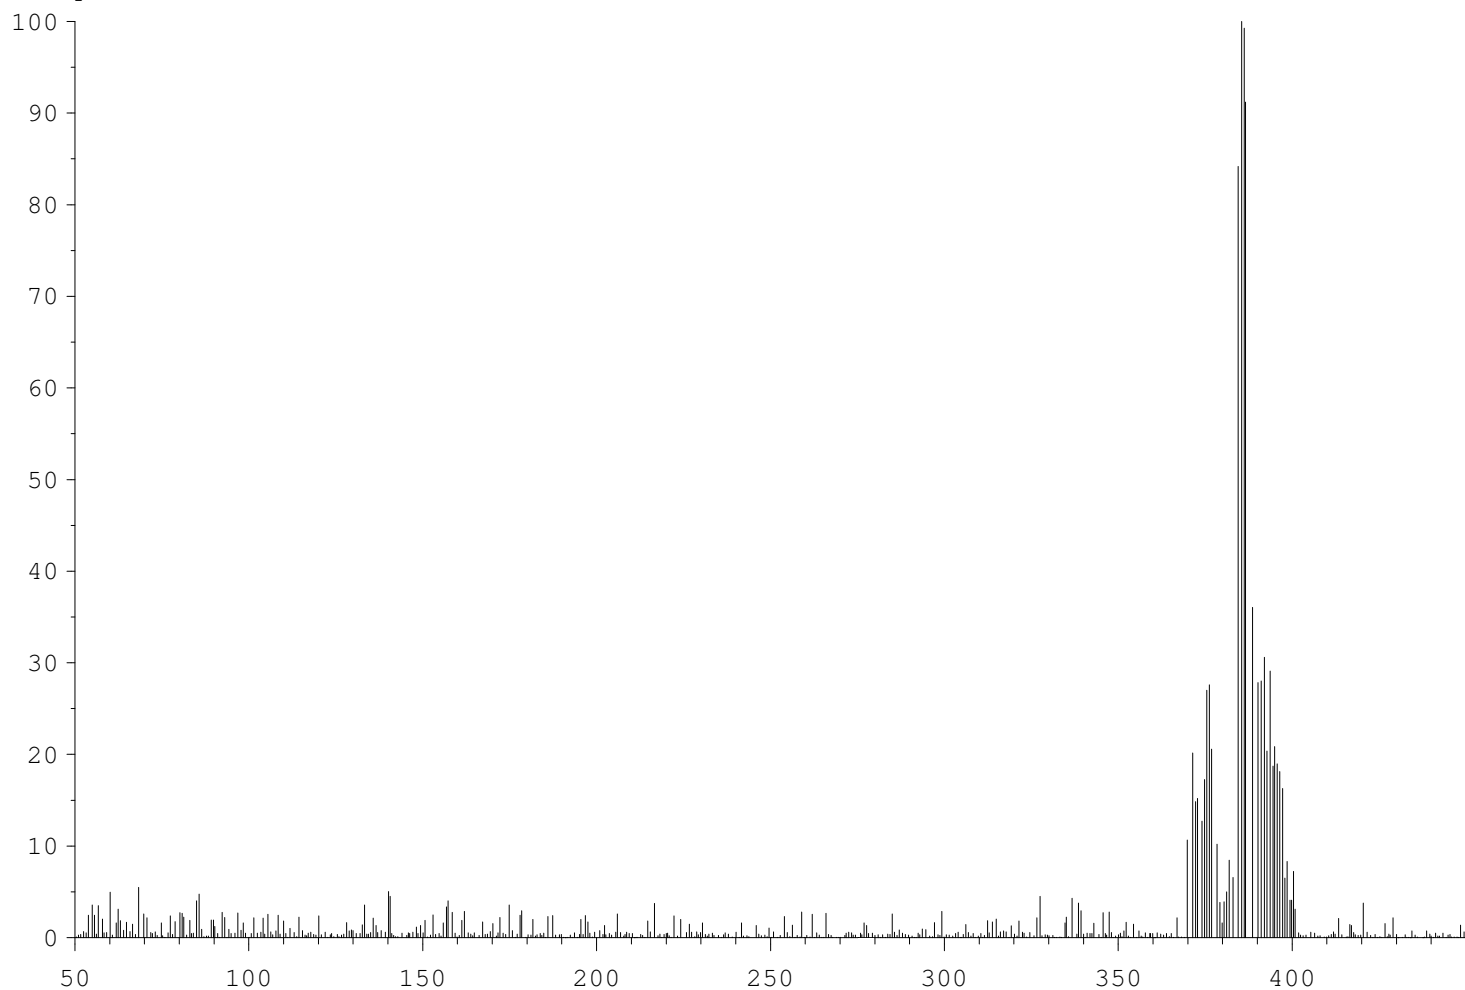

Selected Ion Currents and Detector Gain at EMV = 2447V:

	Mass	I (10 <sup>-16</sup> A)	G (10 <sup>6</sup> )		Mass	I (10 <sup>-16</sup> A)	G (10 <sup>6</sup> )
Acetone	15.0	1.07	1.29	Freon	101.2	1.41	0.70
H2O	17.9	1.56	0.79	Aromat	104.9	0.67	1.08
N2-CO	27.6	1.00	1.09	?	115.0	1.07	0.83
MEOH	31.2	1.16	1.14	?	117.0	0.96	0.75
O2	31.8	1.35	0.93	Aromat	118.8	1.09	0.71
HC-Acet	42.7	1.16	1.00	FC	130.8	0.86	1.04
CO2	44.2	1.21	0.94	HC	141.0	0.78	1.03
IPA	45.1	1.16	0.96	Phthal	148.7	0.84	0.96
Freon	50.7	1.18	0.94	Plsizr	158.7	0.76	1.25
HC	54.8	1.41	0.87	DP Oil	167.9	0.53	1.43
CCH	55.9	1.31	0.76	DP Oil	170.1	0.67	1.31
HC	57.3	0.90	1.08	DP Oil	186.0	0.54	1.24
Acetone	58.3	1.03	1.05	Silcone	206.8	0.73	0.80
IPA	58.7	1.13	1.05	PFTBA	219.0	0.51	1.09
Zn	63.6	0.88	1.23	DP Oil	262.4	0.53	0.89
Zn	66.0	0.89	1.22	Plsizr	276.7	0.55	1.08
HC	67.1	0.88	0.92	DP Oil	278.2	0.74	1.10
HC-Zn	68.0	1.02	0.93	Silcone	280.6	0.69	1.07
HC-FC	69.0	0.72	1.17	Viton	335.9	0.50	0.90
Silcone	73.2	0.95	0.97	DP Oil	354.1	0.57	0.80
HC	76.7	0.98	0.90	Neutral	422.0	0.46	0.94
DCM-CCH	84.0	1.22	0.84	DP Oil	446.3	0.35	1.31
Aromat	91.2	0.92	1.26	Neutral	505.0	0.53	0.91
DP Oil	94.0	0.78	1.22				
Unkwn 1	375.8	11.35	1.66	Unkwn 6	390.8	13.19	1.44
Unkwn 2	384.2	35.43	1.84	Unkwn 7	391.8	11.61	1.55
Unkwn 3	385.4	43.17	1.89	Unkwn 8	393.0	11.64	1.42
Unkwn 4	386.0	41.27	1.89	Unkwn 9	393.5	11.67	1.47
Unkwn 5	386.7	37.22	1.74	Unkwn10	396.0	9.15	1.39